
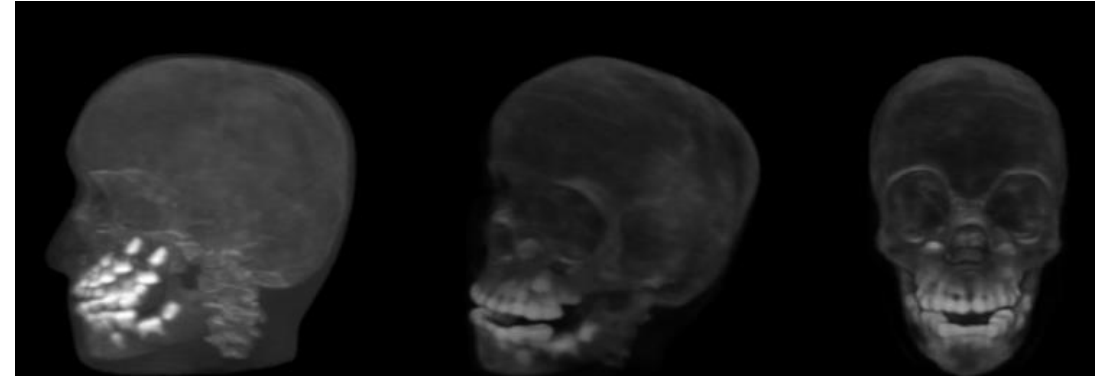


pCT using LGAD (feasibility study)

G. KRAMBERGER

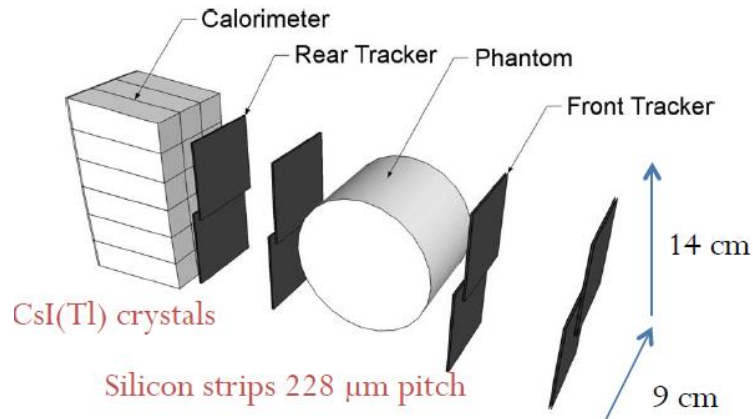


pCT design: summary

Category	Parameter	Value
Proton source	Energy	≈ 200 MeV (head) ≈ 250 MeV (trunk)
	Energy spread	$\approx 0.1\%$
	Beam intensity	$10^3 - 10^7$ protons/sec
Accuracy	Spatial resolution	< 1 mm
	Electron density resolution	$< 1\%$
Time Efficiency	Installation time	< 10 min
	Data acquisition time	< 5 min
	Reconstruction time	< 15 min (treatment planning) < 5 min (dose verification)
Reliability	Detector radiation hardness	> 1000 Gy
	Measurement stability	$< 1\%$
Safety	Maximum dose per scan	< 5 cGy
	Minimum distance to patient surface	10 cm

Measure of x, p, E with $\sigma_x < 1\text{mm}$ $\sigma_E < 1\%$





MHz DAQ :
A head with 100 p, 1 mm voxel
 $7 \cdot 10^8$ p: 10 kHz = 20 hrs
2 MHz = 6 min

GPU reconstruction

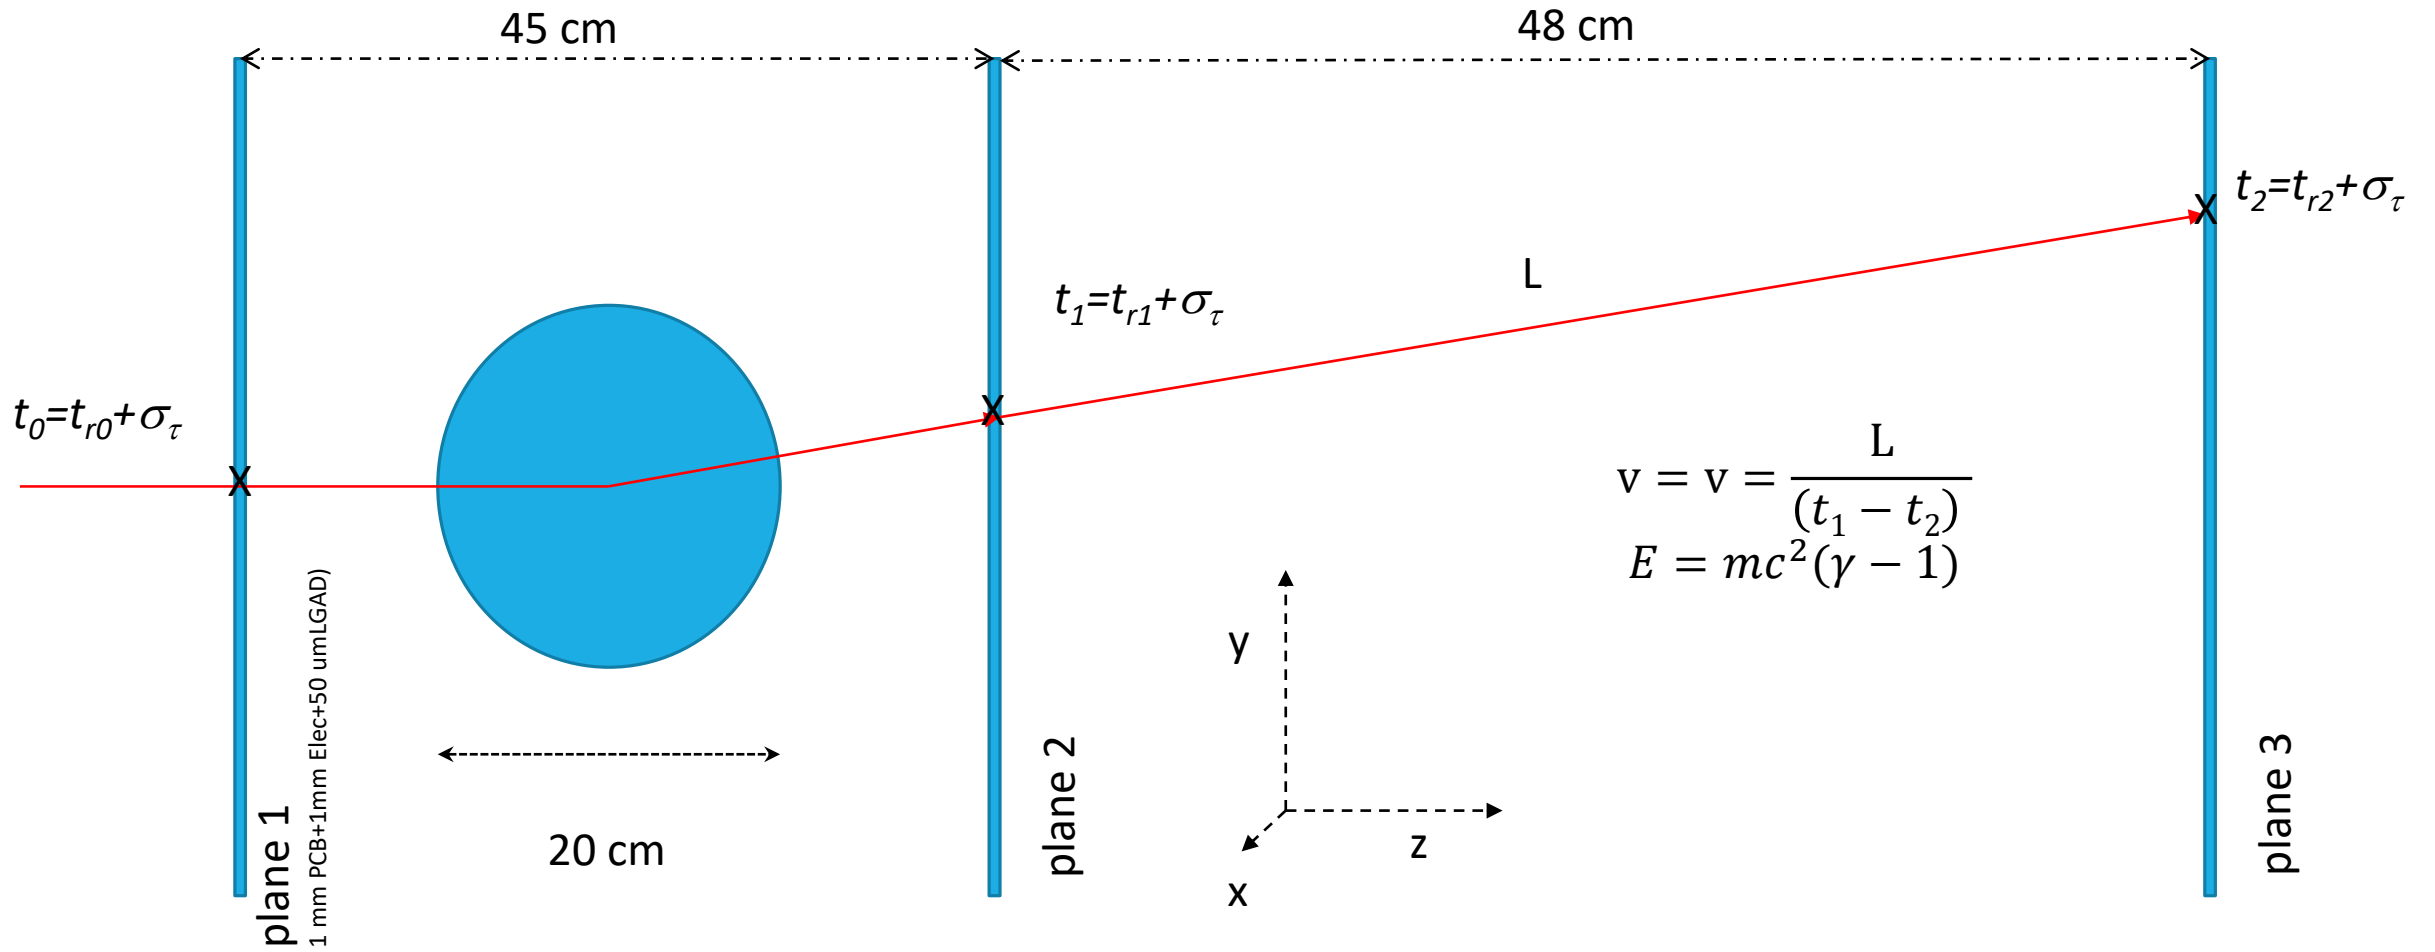

$E_{phantom} = E_p - E_m$
 From $dt = t_0 - t_1$ one can better assume $\rho(r)$



GEANT4 simulations

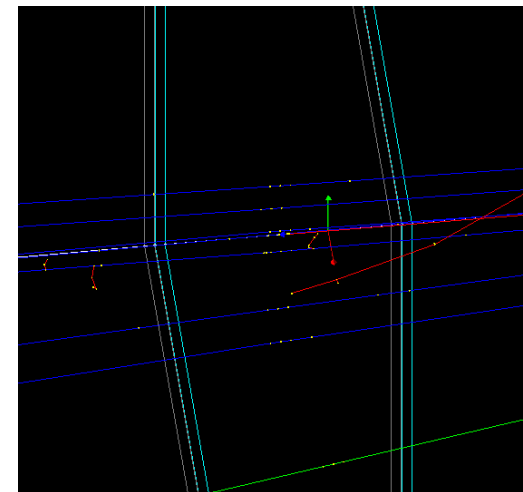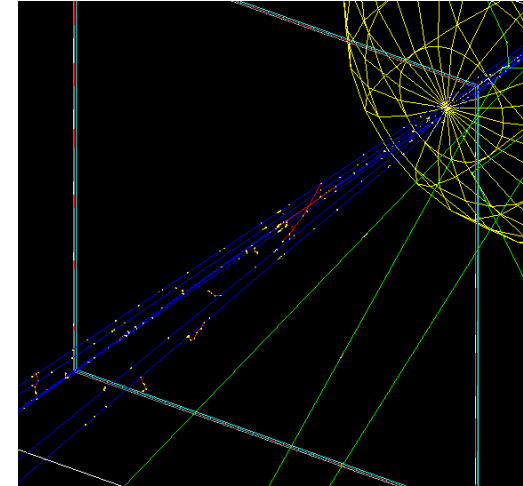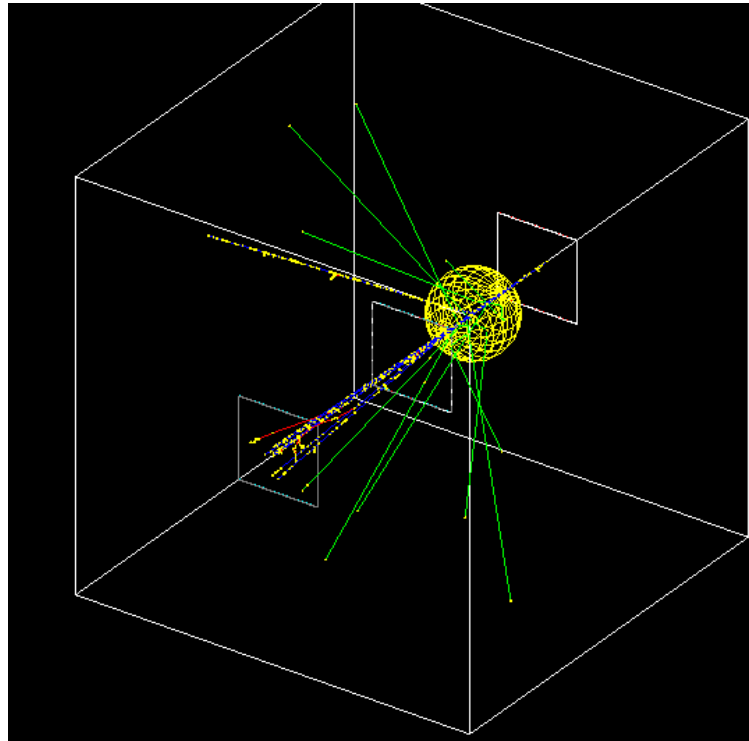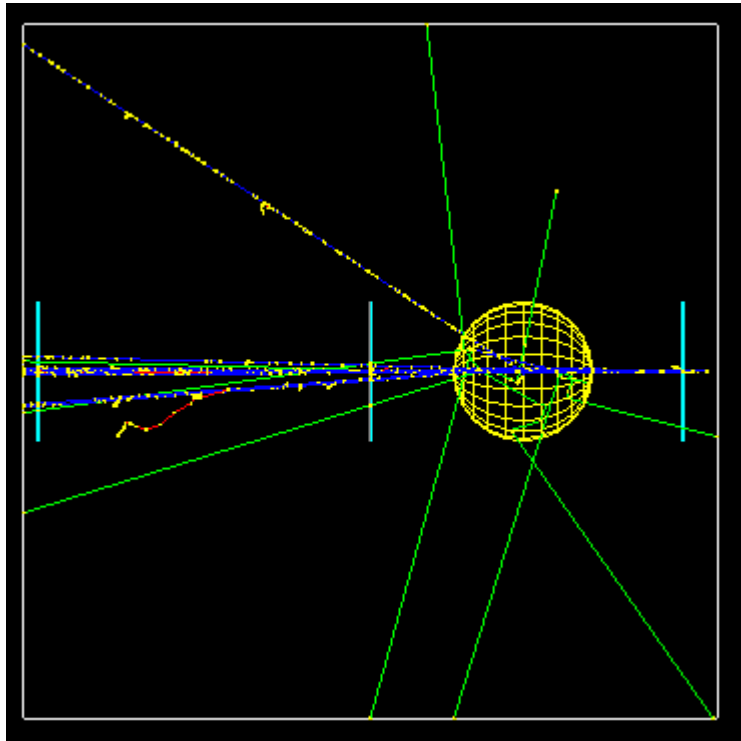

GEANT4 simulations framework done for pCT

What we need is someone who would run this and fully explore the possible benefits of using LGAD !

SIZE OF THE SENSORS

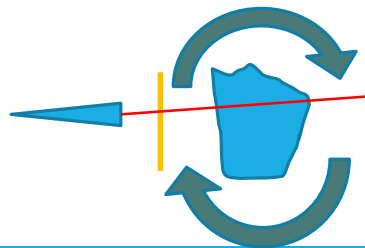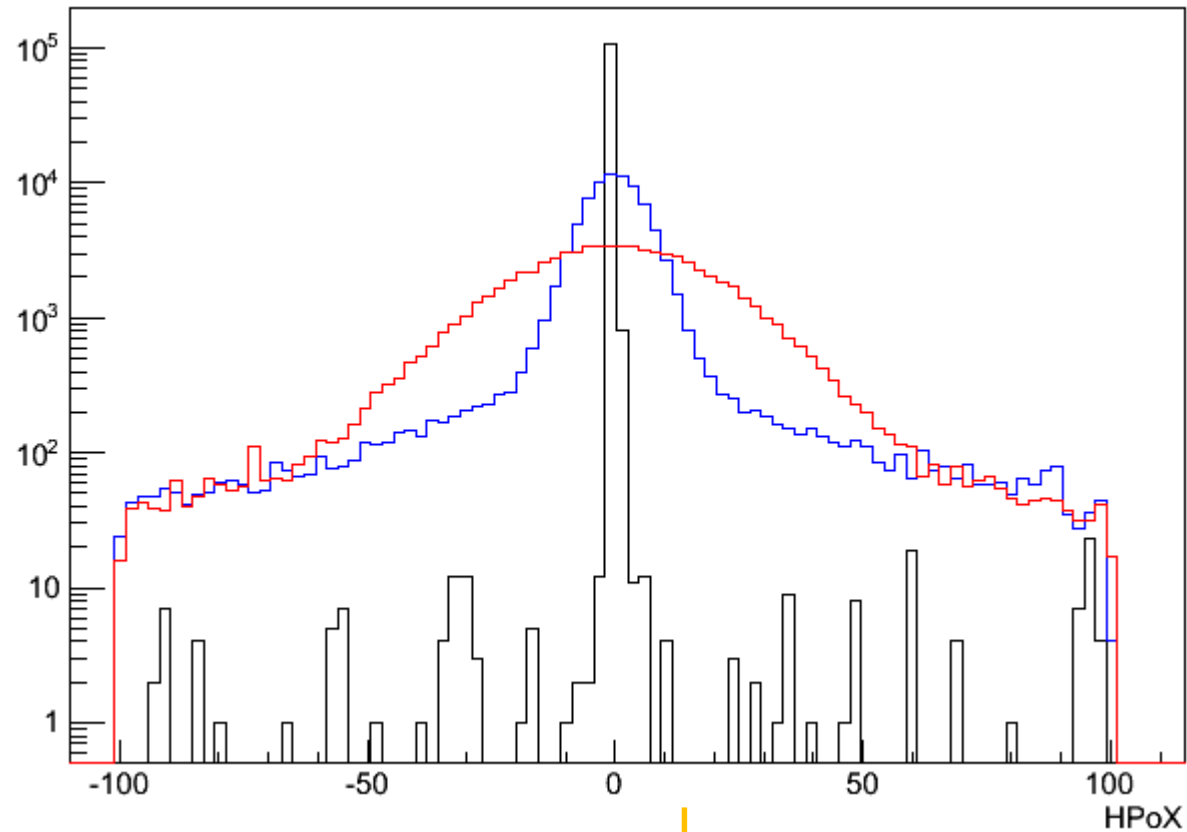

↑
scanning
direction
↓

Large distance between planes require large sensors -> $\sim 10 \times 10$ cm² would be required in the third plane and $\sim 4 \times 4$ cm² in the second and first (maybe even smaller) if realized by scanning.

Different sizes would reduce potential cost.

Head scan required $1e9$ reconstructed p.



Presently most use strip sensors -> hours

Requirement: 10-15 min scan with full reconstruction in an hour

Required DAQ rate > 1 MHz:

- < 1000 μm position resolution is required – lower than 200 μm doesn't help much
- This gives enough floor plan for fast electronics ($\sim 1 \times 1$ mm² pixels – something like ALTIROC)

PROTON ENERGY and DEPOSITED ENERGY

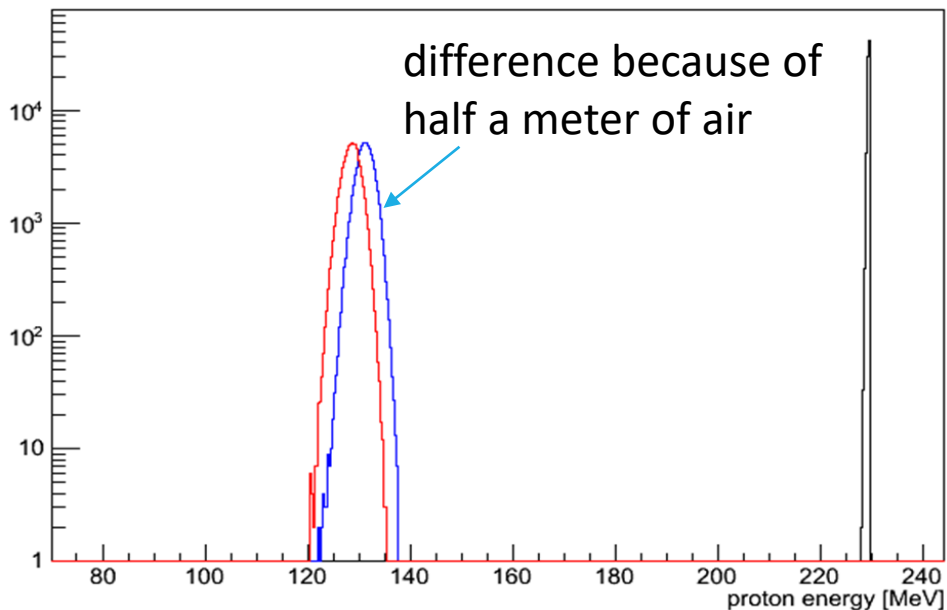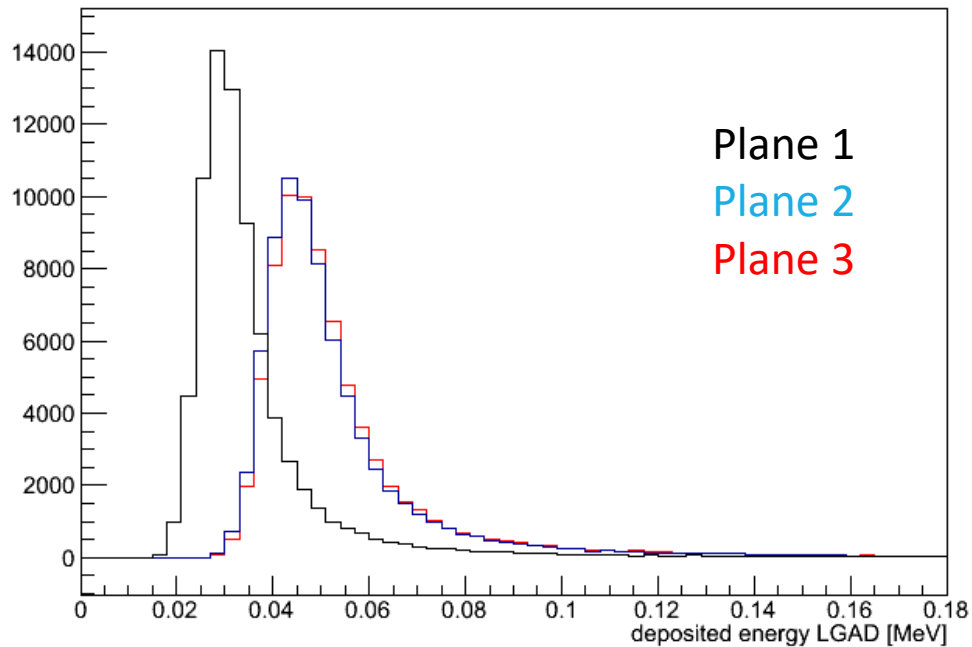



In planes 2 and 3 MPV is around 50 keV (5x larger than for mip)

At a given gain this will improve the time resolution, and allow for 35 um thick LGADs which have been shown to have time resolution of around 20 ps (less Landau fluctuations) with non optimized electronics.


For thin iLGADs for proton detection it is reasonably to assume time resolution of <20 ps

Energy of the protons is reduced by the phantom. This improves the energy resolution as they slow down.

simulated TOF (plane3-plane2)

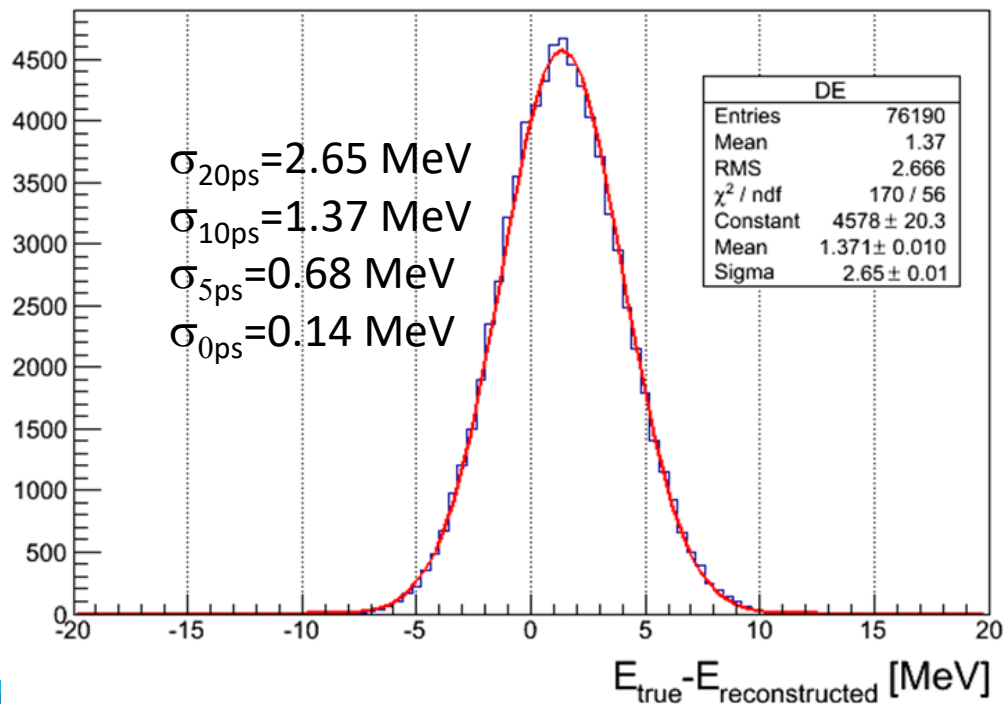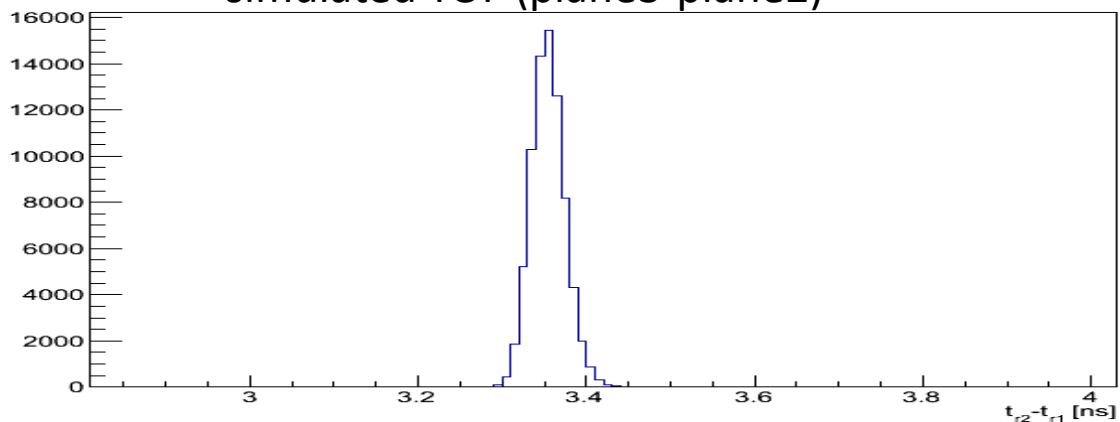

Reconstructed energy


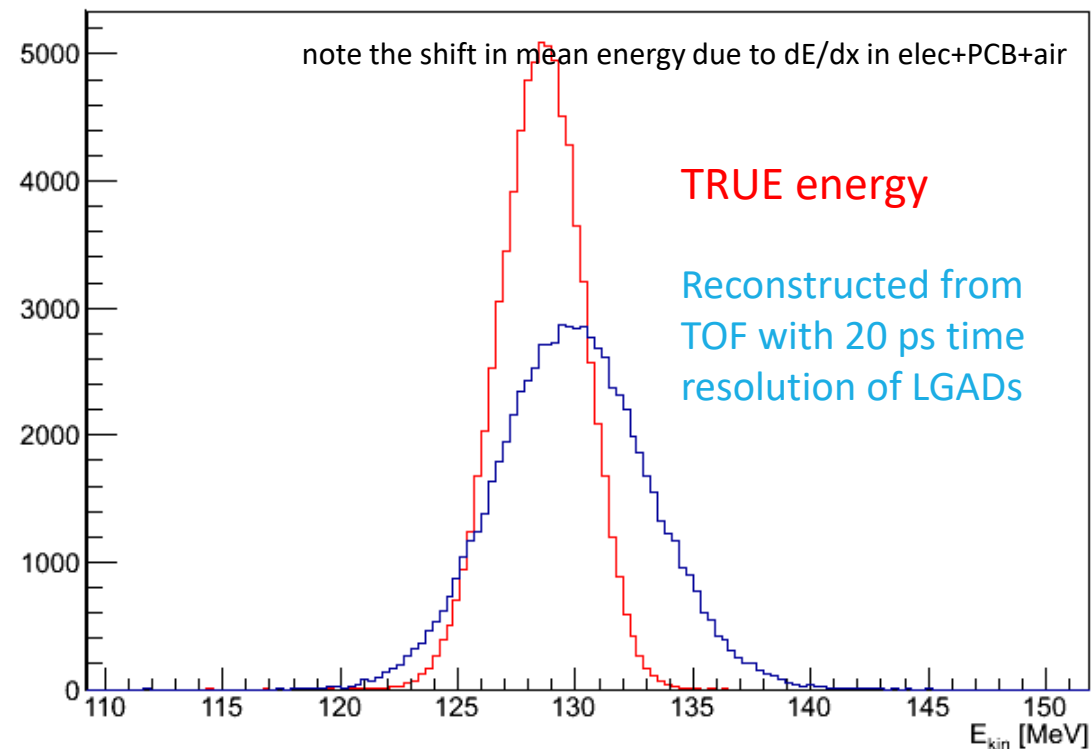


The energy resolution is 2.6 MeV which should be compared to energy resolution of typical CALs !

A drawback is that the energy resolution is a function of the material seen by the beam in the phantom -> a possible solution is using a constraint from the timing information from the first two layers

Better time resolution reduces it even further!

IMPROVED RECONSTRUCTION

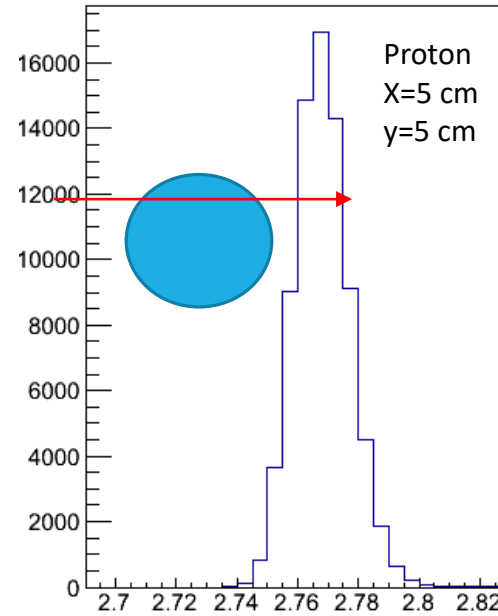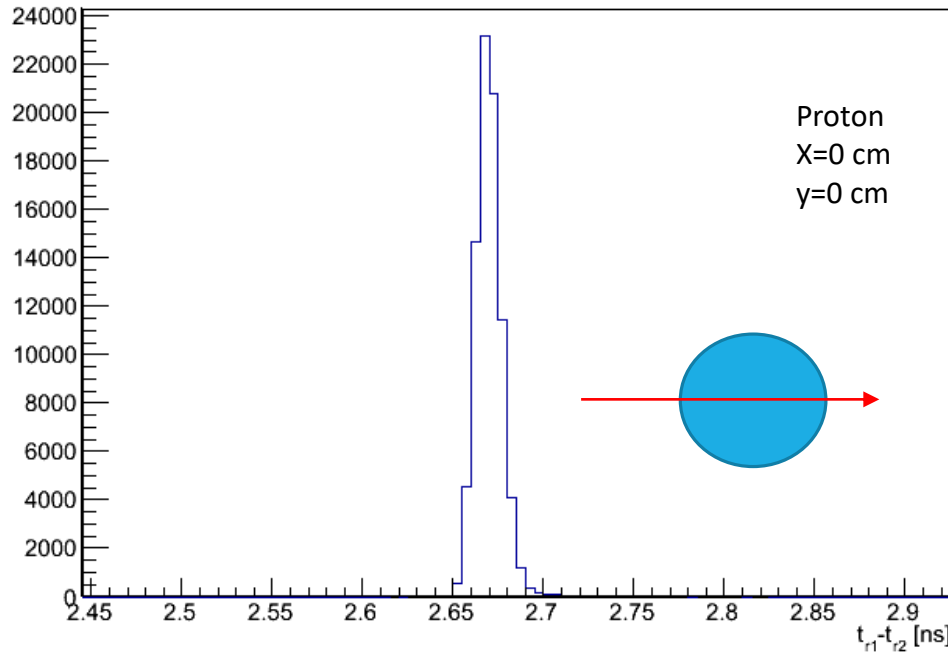



$$\int_L \eta_e(r) dx = \int_{E_{in}}^{E_{out}} \frac{dE}{S_{water}(E)}$$

A difference in time t_1-t_0 can be used to improve MLP calculation -non of the algorithms used so far take this information into account.





Same energy loss and hit position but different $dt=t_0-t_1$
A possible advantage over the conventional pCT and can significantly improve the reconstruction of MPL!

Basically a detector that we have in the lab would do the job – room for improvement is certainly there

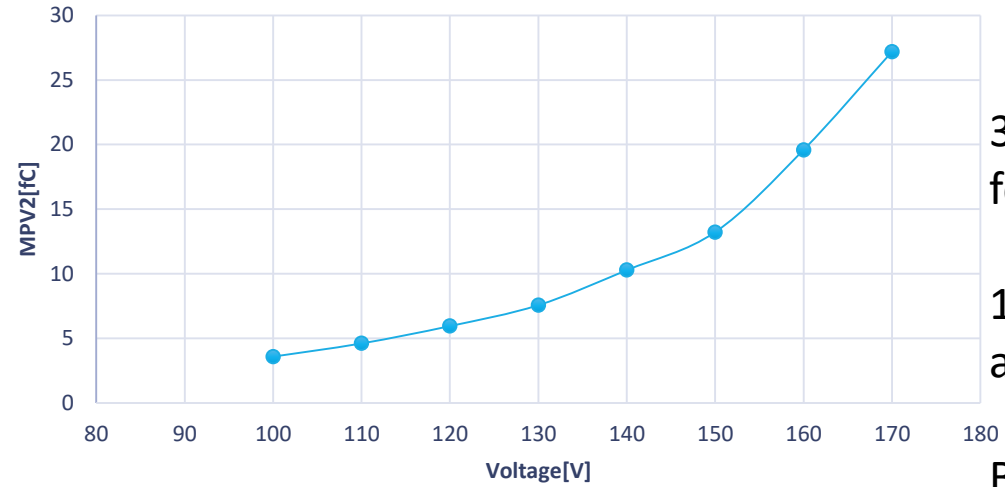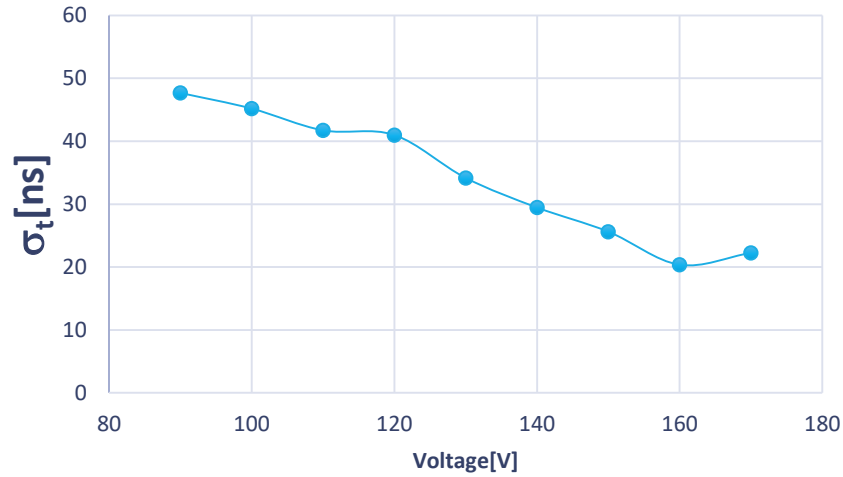

35 um thick LGAD
for ATLAS – HGTD

15x15 arrays
already done

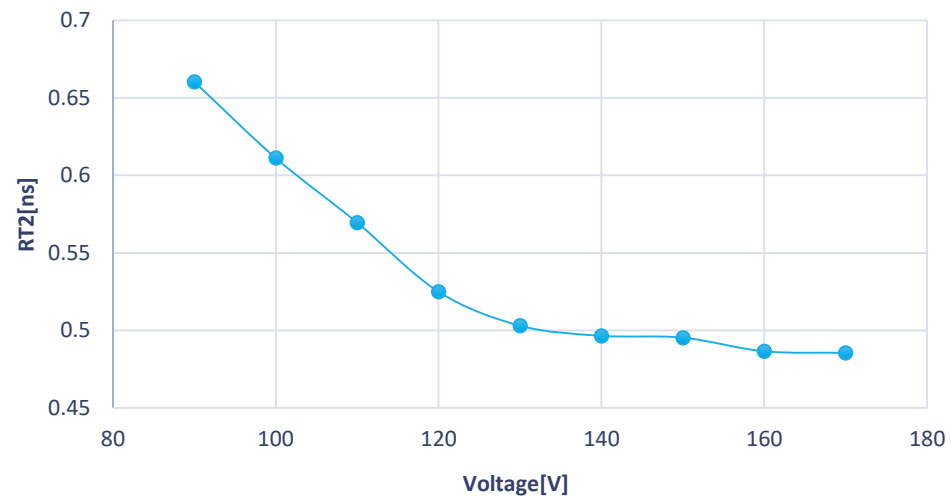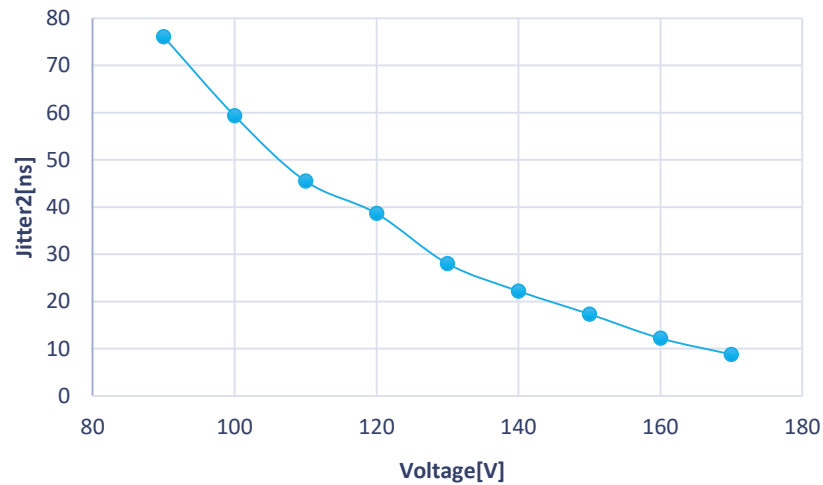

Best achieved so far
in out system
was 18 ps

I think LGADs are ideal detectors for pCT:

- great simplification of the device – no complicated calorimeter needed.
- pixelated LGADs provide good position resolution even with what has been achieved today (ALTIROC)
- iLGAD would be ideal, but with larger pixels also conventional may be good enough (to be checked)
- with improvement of timing resolution to some ~ 15 ps (already achievable on the test bench in our lab) we can achieve energy resolution of 1.5 MeV which is around 1% of the E_p (to be converted to WEP)
- the fact that we have timing information from all three layers allows for better determination of MLP and in combination with other two improve proton energy resolution.
- LGADs are very fast and can easily achieve 1 MHz acquisition rate or even much higher
- the system can be lightweight and can more easily allow for scanning using even smaller modules – say 4×4 cm² in all four planes.

If Slovenia is really going to take part in any form of proton therapy in the future this may be interested for us.