

PQC setup status


IHEP non-irradiated

LCR → Freq = 10 kHz, LVL = 500 mV


LGAD1 IV IV

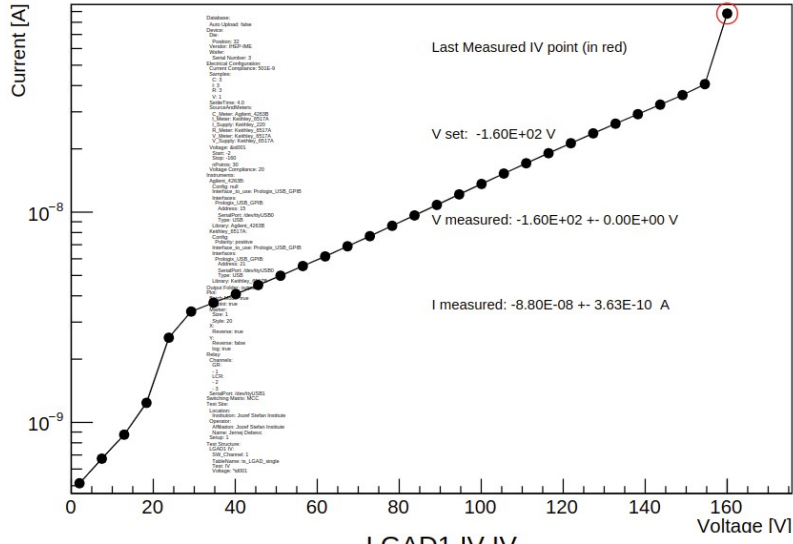


LGAD1 IV IV

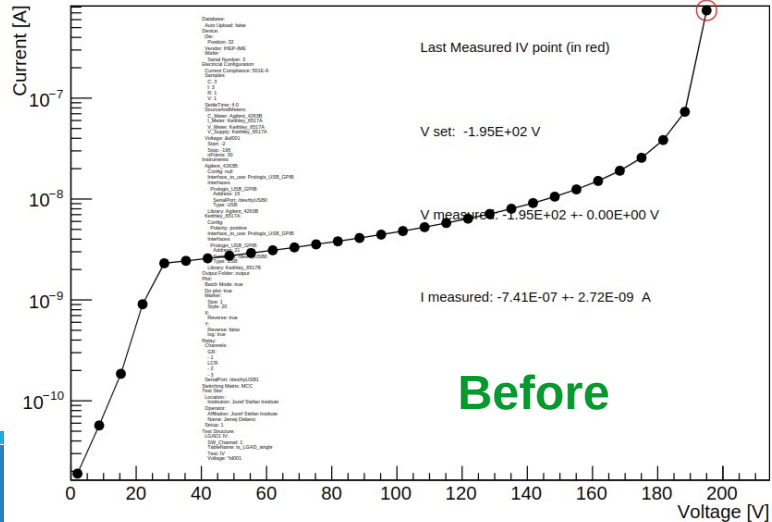


LGAD1 CV CV

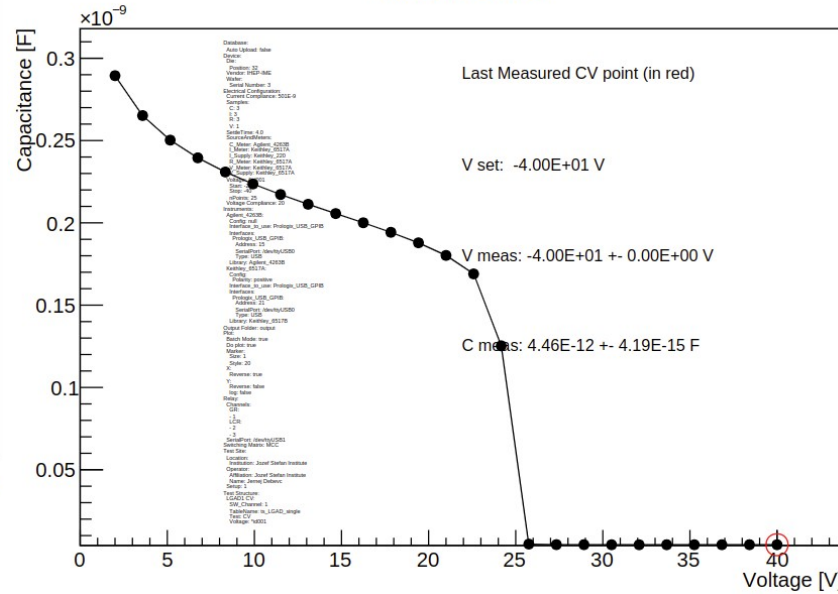

MOS CV CV

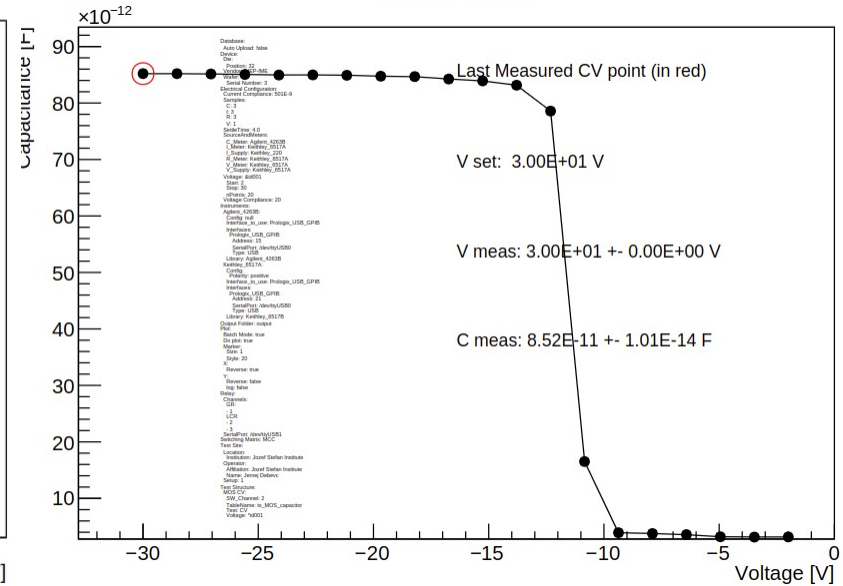

Probe card

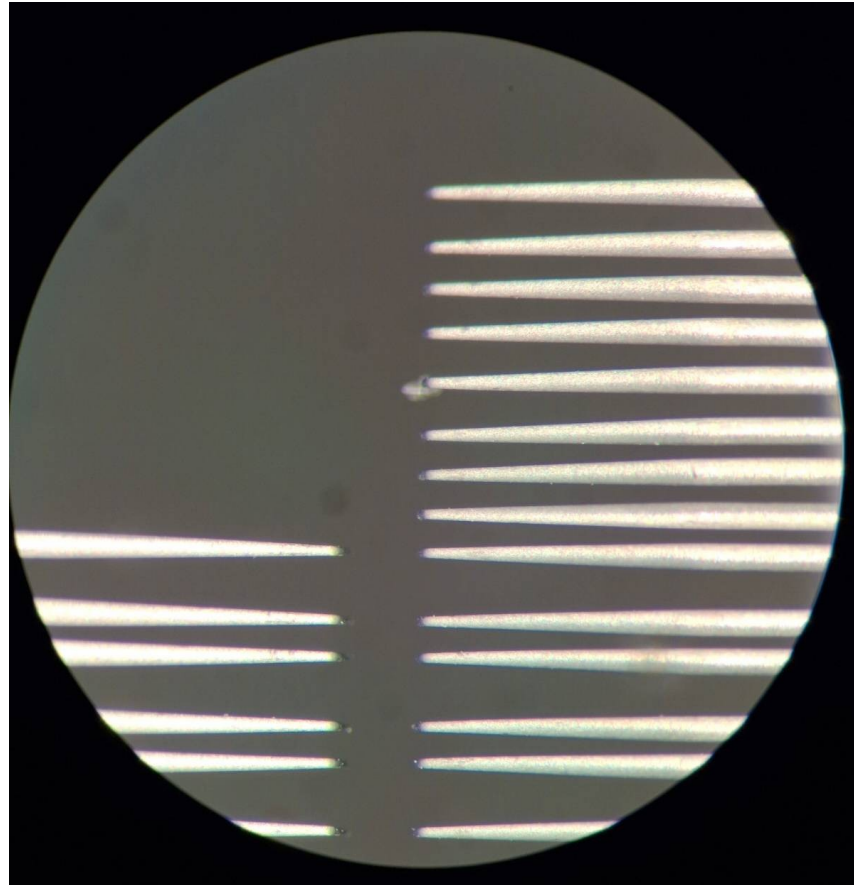

Backup